


# Technical specifications for label creation

# Label template for syringe 3 g (53 x 35 mm)


## Example image



## Printing by external print shop With bleed and crop marks

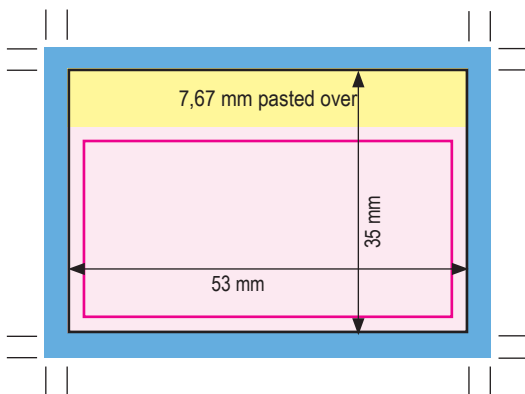

## DMG internal printing With bleed, no crop marks

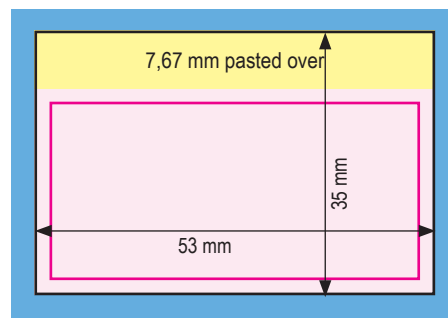

Black border line is for viewing purposes only; please do not create in the data.

Text is at least 2 mm from the edge

Blue border = 3 mm bleed, crop marks

Colors: 4c or Pantone/HKS spot color, please indicate

Black text must be 100% spot black color and overprinted to avoid registration errors and unwanted white edges

Scale symbols correctly

Create print files using Adobe graphic design software

Resolution: 300 dpi

Format: PDF X3 / X4

Black border line is for viewing purposes only; please do not create in the data.

Text is at least 2 mm from the edge

Blue border = 3 mm bleed

Colors: RGB, Pantone/HKS spot color, please indicate

Scale symbols correctly

Create print files using Adobe graphic design software

Resolution: 300 dpi

Format: PDF X3 / X4

## Contents (example size 1:1)

#XXXXXXXX\_X/XX.XXX

DESIGNATION  
Minimum dot size 7 pt.  
Type and color variable

Product name      Contents ml/g  
Type and color

Logo       $xx^{\circ}C$   $xx^{\circ}F$   $xx^{\circ}C$   $xx^{\circ}F$

indigodental GmbH  
Fahltskamp 5  
25421 Pinneberg • Germany  
www.indigodental.com

REF XXXXXXXX      LOT XXXXXXXX  
 MD      i               

LOGO & ADDRESS  
Minimum dot size 4 pt.  
Type and color variable


Adhesive surface

CONTENTS  
(Contents in ml or g | paste | color)  
Minimum dot size 7 pt.  
Type and color variable

ICONS  
Do not change sizes  
Enter reference values (°C|°F)

REF / LOT / Version / Number / Date  
Minimum dot size 5 pt.  
Type and color variable

## Visible areas

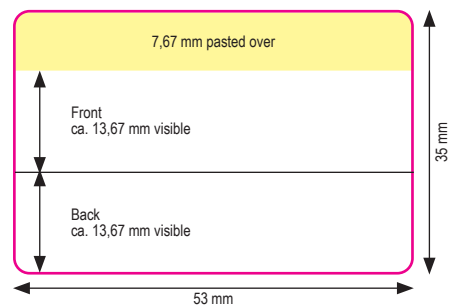

## Icons



(For CE only)  
Minimum height 5 mm